

## Multimodality Imaging in Transcatheter Mitral Interventions Buzzword or Modern Age Toolbox?

Omar K. Khalique, MD; Rebecca T. Hahn, MD

*The secret of change is to focus all of your energy, not on fighting the old, but on building the new.*

—Socrates

Both echocardiography (specifically transesophageal echocardiography [TEE]) and multidetector row computed tomography (MDCT) have played an integral role in preprocedural planning for transcatheter aortic valve replacement, heavily influencing the moniker of “multimodality imaging.” The strengths of each modalities are complementary (Table), although there is overlap between the preprocedural analyses which can be performed.<sup>1,2</sup> Having 2 modalities capable of accurately measuring the same anatomic structure<sup>3</sup> has clinical utility. For instance, mandated MDCT annular measurements could not be performed accurately by the core laboratory in 6% to 8% of patients in the Placement of Aortic Transcatheter Valves II SAPIEN 3 trial<sup>4</sup> and thus required 3-dimensional (3D)-TEE for transcatheter valve sizing.

### See Articles by Suh et al and Mak et al

Perhaps, the most important imaging lesson learned from the transcatheter aortic valve replacement (TAVR) experience is not whether one modality is better or worse than another, but the fact that because of the obvious utility of multiple imaging modalities, the imager has become an essential part of the Heart Team and integral to the preprocedural and intraprocedural planning for any successful transcatheter device implantation.<sup>5,6</sup> The imager must have a comprehensive understanding of the anatomy of interest, as well as the intended transcatheter device. Without this knowledge, recommendations for sizing and positioning, as well as anticipation of complications, are not possible. At our institution, review of both MDCT and echocardiographic imaging is part of the initial patient assessment. In addition, an imager is always present for all structural heart disease interventions, allowing the interventionalist or surgeon and the imager to gain experience together. Mutual respect is key to this learning process.

The opinions expressed in this article are not necessarily those of the editors or of the American Heart Association.

From the Department of Medicine, Division of Cardiology, Columbia University Medical Center/New York Presbyterian Hospital, New York, NY.

Correspondence to Rebecca T. Hahn, MD, Columbia University Medical Center, New York Presbyterian Hospital, 177 Fort Washington Ave, New York, NY 10032. E-mail [rh2@columbia.edu](mailto:rh2@columbia.edu)

(*Circ Cardiovasc Imaging*. 2016;9:e005071.)

DOI: 10.1161/CIRCIMAGING.116.005071.)

© 2016 American Heart Association, Inc.

*Circ Cardiovasc Imaging* is available at  
<http://circimaging.ahajournals.org>

DOI: 10.1161/CIRCIMAGING.116.005071

Transcatheter mitral interventions have largely been discussed in the context of percutaneous edge-to-edge repair with the MitraClip (Abbott Vascular, CA) for mitral regurgitation. TEE has been essential from the inception of the device, with desirable outcomes attributed to imaging guidance.<sup>7,8</sup> Since that time, the role of 3D-TEE in detailed imaging assessment of not only mitral regurgitant severity but also complex mitral anatomic details has become indisputable.<sup>9</sup>

As we enter the next phase of transcatheter mitral valve interventions of new repair and replacement devices as well as standardization of transcatheter paravalvular leak (PVL) closure, the role of imaging is evolving. MDCT and 3D-TEE are currently being used to screen patients anatomically for transcatheter mitral valve replacement. Real-time 3D-TEE has been integral to our understanding of the dynamic nature of the mitral valve complex in normal patients, as well primary and secondary mitral valve disease.<sup>10–14</sup> Screening methods for transcatheter mitral valve replacement have been largely undefined because of the lack of experience in this field and the confidentiality of early feasibility studies. The idea of the D-shaped annulus has been popularized in recent literature as a method to measure the mitral annulus, which simplifies the annulus shape while making it more planar; this is also partially based on the observation that the anterior saddle as a portion of the annulus measurement projects past the anterior mitral leaflet into the left ventricular outflow tract.<sup>15</sup> As a continuation of these investigations, Mak et al,<sup>16</sup> in this issue of *Circulation: Cardiovascular Imaging*, use the Mitral Valve Quantification program (Philips Healthcare, Inc., Andover, MA) in a modified fashion to perform a D-shaped segmentation of the mitral annulus using 3D-TEE similar to the same group's original method on a semiautomated MDCT software segmentation. In this analysis of 41 patients, annular area and circumference, were not different when comparing MDCT and 3D-TEE measurements. Correlation between modalities was also strong. The current study importantly highlights the ability to interchangeably use MDCT and 3D-TEE for mitral annulus sizing early in the experience. More specifically, the study emphasizes using similar methodology across both modalities to achieve these results rather than incorrectly comparing incongruous methods, as was done early with many aortic annulus publications which compared 3-dimensional MDCT measurements to 2-dimensional echocardiographic measurements. Although the D-shaped model developed by Blanke et al appears to mimic the nature of the mitral annulus at the hinge point of the anterior leaflet, it is unclear at this early stage whether this is the best method of measurement before transcatheter mitral replacement. The aortic–mitral continuity is a complex portion of the saddle-shaped structure of the annulus, and this area bows to and fro throughout the

**Table. Advantages and Limitations of Imaging Modalities for Structural Heart Disease Interventions**


Imaging Modality	Advantages	Disadvantages
MDCT	Comprehensive cardiac and vascular assessment Blood–tissue interface well-defined Calcium well imaged/quantified High reproducibility Noninvasive	Artifacts of imaging Iodinated contrast requirement Radiation exposure Cardiac cycle–dependent Poor temporal resolution on most systems
TEE	High temporal resolution Pulsed, continuous, and color-flow Doppler Real-time/multibeam imaging High safety profile of ultrasound No contrast required Portable	Semi-invasive Acoustic shadowing and other artifacts of imaging Higher operator dependence

MDCT indicates multidetector row computed tomography; and TEE, transesophageal echocardiography.

cardiac cycle (Figure). The impact of this phenomenon on sizing of transcatheter mitral valves is unclear. All of the analyses by Mak et al<sup>16</sup> were performed in diastole, where typically the annulus plane is easier to appreciate. However, existing studies of mitral annular dynamism based on 3D-TEE have shown the largest dimensions in late systole.<sup>12,17,18</sup> Systolic annular measurements are more challenging in the setting of closed mitral leaflets, where the hinge points may not be easily discerned. It stands to reason that there may be a significant impact of leaflet dynamics and anatomy on seating of transcatheter mitral devices, which has yet to be defined. Although an early comparative study by Shanks et al<sup>19</sup> showed excellent agreement between MDCT and 3D-TEE for mitral annular measurements as well as leaflet morphology, until MDCT analysis of leaflet morphology can be consistently duplicated, detailed leaflet analysis falls clearly into the realm of echocardiography. Left ventricular outflow tract obstruction, on the contrary, is an additional concern in transcatheter mitral replacement; measurement of a neo-left ventricular outflow tract which is formed by the displacement of the anterior mitral leaflet by the transcatheter mitral valve is easily performed on MDCT.

In this same issue, Suh et al<sup>20</sup> compare MDCT to transthoracic echocardiography and 2-dimensional (2D) TEE analysis of mitral PVL severity and location. In 78 patients who had undergone reoperation, MDCT had a not surprisingly better (although not statistically significant) diagnostic accuracy for detection of PVL. MDCT had a similar diagnostic accuracy for detection of PVL to 2D-TEE. The authors should be congratulated on the efforts to push the limits of the diagnostic abilities of MDCT. The correlation between PVL severity planimeted by MDCT and assessed by 2D-TEE methods was statistically significant but weak. Imaging quality for MDCT was nondiagnostic in 12/204 patients due to beam-hardening artifacts, all in mechanical valves.

The use of 2D-TEE imaging, however, is a significant limitation of this study. Real-time 3D-TEE has been used extensively during percutaneous PVL closure procedures<sup>21–23</sup> and can depict not only the relevant cardiac landmarks adjacent to the sites of PVLs, but also wires, delivery catheters, and closure devices.<sup>24</sup> Real-time 3D-TEE imaging results in a more accurate localization of paravalvular defects and an estimation of the size of the defect that correlates better with surgical findings when compared with 2D-TEE.<sup>25</sup> Thus, one would expect better correlation between 3D-TEE multiplanar reconstruction with or without color Doppler, to MDCT planimetry of paravalvular defects. The analysis begs the question of what additional benefits MDCT provides over TEE if intraoperative 3D-TEE guidance will be used for closure of leaks. Patient preference is a significant consideration in the preprocedural assessment; however, further cost-benefit as well as accuracy studies may be needed before recommending MDCT as an equivalent technology to 3D echocardiography for mitral PVL assessment. A greater argument could be made for the use of MDCT for the assessment of aortic PVLs, where acoustically shadowing of distal structures may mask PVL. Again, one cannot ignore the potential harm of MDCT radiation and iodinated contrast which must be balanced against the benefits. Coregistration is another

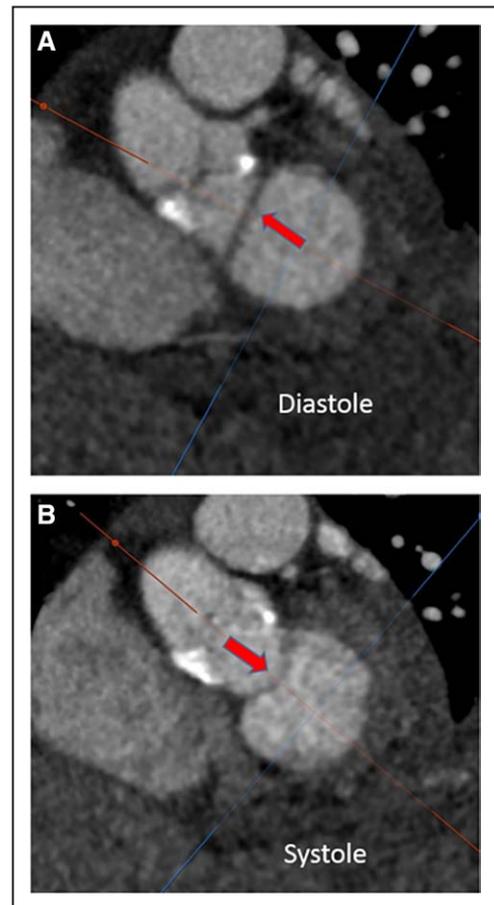

**Figure.** The aortic–mitral continuity. The inflow and outflow regions of the left heart are in direct continuity. The aortic–mitral continuity is a complex, dynamic portion of the saddle-shaped structure of the mitral annulus, which changes shape from diastole (A) to systole (B).

technology in its early stages, which may add more value to MDCT preprocedural planning; however, similar coregistration can be performed with intraprocedural 3D-TEE.<sup>26</sup> Nonetheless, imaging advancements in MDCT spatial resolution and reconstruction techniques which have made this discussion possible are truly exciting.

As if all of the challenges outlined above were not enough, an additional challenge arises after devices are placed. Native mitral valve regurgitation assessment by echocardiography is well established. Methods of assessment include quantitative Doppler and direct planimetry of effective regurgitant orifice area by 3D reconstruction.<sup>27,28</sup> However, after transcatheter devices are placed, these methods become less accurate or invalid because of Doppler flow acceleration and acoustic artifacts from devices. In the post-transcatheter edge-to-edge repair setting, multiple mitral regurgitation jets may be difficult to assess on TEE color Doppler imaging because of artifacts from the device(s). Additionally, if jets are entrained by the devices, excessive jet spray could cause an overestimation of mitral regurgitant severity. Following MitraClip, assessment of residual regurgitation can be assessed by 3D color Doppler.<sup>29</sup> Cardiac magnetic resonance (CMR) is also promising in the assessment of regurgitant volume by both volumetric and velocity-encoding methods, showing excellent reproducibility in the post MitraClip setting.<sup>30</sup> CMR has shown prognostic value in diagnosing PVL after transcatheter aortic valve replacement.<sup>31</sup> A promising area of further study would be the similar utility to measure mitral regurgitant volumes after mitral PVL closure or after transcatheter mitral valve replacement. Although often used as the gold standard for volumetric measurement, CMR suffers from motion, arrhythmia gating, and magnetic artifacts from metal-containing prostheses. Additionally, there is often the question of consistency of application of measuring the basal slice for inclusion in volumetric measurements.<sup>32</sup> Magnetic distortion from a mitral prosthesis (whether surgical or transcatheter) may be a particularly problematic artifact in the basal slice depending on the patient. Nonetheless, CMR consistently shows excellent reproducibility and may be the best option for overall quantification. When carefully performed, 3D-transsthoracic echocardiography has been shown to have similarly excellent reproducibility to CMR<sup>33</sup> and could theoretically be used to calculate regurgitant volumes as well, with the considerations of acoustic artifacts from prostheses. Luckily, we do not have to depend only on one modality.

We are fortunate to have multimodality imaging available as a true modern-day toolbox. As both Mak et al<sup>16</sup> and Suh et al<sup>20</sup> have shown, advances in imaging technology result in multiple imaging options, which allow us to best assess our patients. This will be crucial not only in structural interventions but in other areas of cardiology. It is up to us to leverage these technologies and use our collective expertise to drive the field forward to obtain the best outcomes for our patients.

## Disclosures

None.

## References

- Achenbach S, Delgado V, Hausleiter J, Schoenhagen P, Min JK, Leipsic JA. SCCT expert consensus document on computed tomography imaging before transcatheter aortic valve implantation (TAVI)/transcatheter aortic valve replacement (TAVR). *J Cardiovasc Comput Tomogr*. 2012;6:366–380. doi: 10.1016/j.jcct.2012.11.002.
- Hahn RT, Little SH, Monaghan MJ, Kodali SK, Williams M, Leon MB, Gillam LD. Recommendations for comprehensive intraprocedural echocardiographic imaging during TAVR. *JACC Cardiovasc Imaging*. 2015;8:261–287. doi: 10.1016/j.jcmg.2014.12.014.
- Khalique OK, Kodali SK, Paradis JM, Nazif TM, Williams MR, Einstein AJ, Pearson GD, Harjai K, Grubb K, George I, Leon MB, Hahn RT. Aortic annular sizing using a novel 3-dimensional echocardiographic method: use and comparison with cardiac computed tomography. *Circ Cardiovasc Imaging*. 2014;7:155–163. doi: 10.1161/CIRCIMAGING.113.001153.
- Thourani VH, Kodali S, Makkar RR, Herrmann HC, Williams M, Babaliaros V, Smalling R, Lim S, Malaisrie SC, Kapadia S, Szeto WY, Greason KL, Kereiakes D, Ailawadi G, Whisenant BK, Devireddy C, Leipsic J, Hahn RT, Pibarot P, Weissman NJ, Jaber WA, Cohen DJ, Suri R, Tuzcu EM, Svensson LG, Webb JG, Moses JW, Mack MJ, Miller DC, Smith CR, Alu MC, Parvataneni R, D'Agostino RB Jr, Leon MB. Transcatheter aortic valve replacement versus surgical valve replacement in intermediate-risk patients: a propensity score analysis. *Lancet*. 2016;387:2218–2225. doi:10.1016/S0140-6736(16)30073-3.
- Holmes DR Jr, Mack MJ, Kaul S, Agnihotri A, Alexander KP, Bailey SR, Calhoun JH, Carabello BA, Desai MY, Edwards FH, Francis GS, Gardner TJ, Kappetein AP, Linderbaum JA, Mukherjee C, Mukherjee D, Otto CM, Ruiz CE, Sacco RL, Smith D, Thomas JD. 2012 ACCF/AATS/SCAI/STS expert consensus document on transcatheter aortic valve replacement. *J Am Coll Cardiol*. 2012;59:1200–1254. doi: 10.1016/j.jacc.2012.01.001.
- Nishimura RA, Otto CM, Bonow RO, Carabello BA, Erwin JP III, Guyton RA, O'Gara PT, Ruiz CE, Skubas NJ, Sorajja P, Sundt TM III, Thomas JD; American College of Cardiology/American Heart Association Task Force on Practice Guidelines. 2014 AHA/ACC guideline for the management of patients with valvular heart disease: executive summary: a report of the American College of Cardiology/American Heart Association Task Force on Practice Guidelines. *J Am Coll Cardiol*. 2014;63:2438–2488. doi: 10.1016/j.jacc.2014.02.537.
- Silvestry FE, Rodriguez LL, Herrmann HC, Rohatgi S, Weiss SJ, Stewart WJ, Homma S, Goyal N, Pulerwitz T, Zunamon A, Hamilton A, Merlino J, Martin R, Krabill K, Block PC, Whitlow P, Tuzcu EM, Kapadia S, Gray WA, Reisman M, Wasserman H, Schwartz A, Foster E, Feldman T, Wieggers SE. Echocardiographic guidance and assessment of percutaneous repair for mitral regurgitation with the Evalve MitraClip: lessons learned from EVEREST I. *J Am Soc Echocardiogr*. 2007;20:1131–1140. doi: 10.1016/j.echo.2007.02.003.
- Feldman T, Foster E, Glower DD, Glower DG, Kar S, Rinaldi MJ, Fail PS, Smalling RW, Siegel R, Rose GA, Engeron E, Loghini C, Trento A, Skipper ER, Fudge T, Letsou GV, Massaro JM, Mauri L; EVEREST II Investigators. Percutaneous repair or surgery for mitral regurgitation. *N Engl J Med*. 2011;364:1395–1406. doi: 10.1056/NEJMoa1009355.
- Tsang W, Lang RM. Three-dimensional echocardiography is essential for intraoperative assessment of mitral regurgitation. *Circulation*. 2013;128:643–652. doi: 10.1161/CIRCULATIONAHA.112.120501.
- Levine RA, Handschumacher MD, Sanfilippo AJ, Hagege AA, Harrigan P, Marshall JE, Weyman AE. Three-dimensional echocardiographic reconstruction of the mitral valve, with implications for the diagnosis of mitral valve prolapse. *Circulation*. 1989;80:589–598.
- Topilsky Y, Vaturi O, Watanabe N, Bichara V, Nkomo VT, Michelena H, Le Tourneau T, Mankad SV, Park S, Capps MA, Suri R, Pislaru SV, Maalouf J, Yoshida K, Enriquez-Sarano M. Real-time 3-dimensional dynamics of functional mitral regurgitation: a prospective quantitative and mechanistic study. *J Am Heart Assoc*. 2013;2:e000039. doi: 10.1161/JAHA.113.000039.
- Grewal J, Suri R, Mankad S, Tanaka A, Mahoney DW, Schaff HV, Miller FA, Enriquez-Sarano M. Mitral annular dynamics in myxomatous valve disease: new insights with real-time 3-dimensional echocardiography. *Circulation*. 2010;121:1423–1431. doi: 10.1161/CIRCULATIONAHA.109.901181.
- Watanabe N, Ogasawara Y, Yamaura Y, Wada N, Kawamoto T, Toyota E, Akasaka T, Yoshida K. Mitral annulus flattens in ischemic mitral regurgitation: geometric differences between inferior and anterior myocardial infarction: a real-time 3-dimensional echocardiographic study. *Circulation*. 2005;112(9 suppl):I458–I462. doi: 10.1161/CIRCULATIONAHA.104.524595.

14. Zeng X, Nunes MC, Dent J, Gillam L, Mathew JP, Gammie JS, Ascheim DD, Moquete E, Hung J. Asymmetric versus symmetric tethering patterns in ischemic mitral regurgitation: geometric differences from three-dimensional transesophageal echocardiography. *J Am Soc Echocardiogr.* 2014;27:367–375. doi: 10.1016/j.echo.2014.01.006.
15. Blanke P, Dvir D, Cheung A, Ye J, Levine RA, Precious B, Berger A, Stub D, Hague C, Murphy D, Thompson C, Munt B, Moss R, Boone R, Wood D, Pache G, Webb J, Leipsic J. A simplified D-shaped model of the mitral annulus to facilitate CT-based sizing before transcatheter mitral valve implantation. *J Cardiovasc Comput Tomogr.* 2014;8:459–467. doi: 10.1016/j.jcct.2014.09.009.
16. Mak GJ, Blanke P, Ong K, Naoum C, Thompson CR, Webb JG, Moss R, Boone R, Ye J, Cheung A, Munt B, Leipsic J, Grewal J. Three-dimensional echocardiography compared with computed tomography to determine mitral annulus size before transcatheter mitral valve implantation. *Circ Cardiovasc Imaging.* 2016;9:e004176. doi: 10.1161/CIRCIMAGING.115.004176.
17. Kwan J, Jeon MJ, Kim DH, Park KS, Lee WH. Does the mitral annulus shrink or enlarge during systole? A real-time 3D echocardiography study. *J Korean Med Sci.* 2009;24:203–208. doi: 10.3346/jkms.2009.24.2.203.
18. Khabbaz KR, Mahmood F, Shakil O, Warraich HJ, Gorman JH 3rd, Gorman RC, Matyal R, Panzica P, Hess PE. Dynamic 3-dimensional echocardiographic assessment of mitral annular geometry in patients with functional mitral regurgitation. *Ann Thorac Surg.* 2013;95:105–110. doi: 10.1016/j.athoracsur.2012.08.078.
19. Shanks M, Delgado V, Ng AC, van der Kleij F, Schuijff JD, Boersma E, van de Veire NR, Nucifora G, Bertini M, de Roos A, Kroft L, Schalij MJ, Bax JJ. Mitral valve morphology assessment: three-dimensional transesophageal echocardiography versus computed tomography. *Ann Thorac Surg.* 2010;90:1922–1929. doi: 10.1016/j.athoracsur.2010.06.116.
20. Suh YJ, Hong G-R, Han K, Im DJ, Chang S, Hong YJ, Lee H-J, Hur J, Choi BW, Chang B-C, Shim CY, Kim YJ. Assessment of mitral paravalvular leakage after mitral valve replacement using cardiac computed tomography: comparison with surgical findings. *Circ Cardiovasc Imaging.* 2016;9:e004153. doi: 10.1161/CIRCIMAGING.115.004153.
21. Rihal CS, Sorajja P, Booker JD, Hagler DJ, Cabalka AK. Principles of percutaneous paravalvular leak closure. *JACC Cardiovasc Interv.* 2012;5:121–130. doi: 10.1016/j.jcin.2011.11.007.
22. Ruiz CE, Jelmin V, Kronzon I, Dudiy Y, Del Valle-Fernandez R, Einhorn BN, Chiam PT, Martinez C, Eiros R, Roubin G, Cohen HA. Clinical outcomes in patients undergoing percutaneous closure of periprosthetic paravalvular leaks. *J Am Coll Cardiol.* 2011;58:2210–2217. doi: 10.1016/j.jacc.2011.03.074.
23. Nietlispach F, Johnson M, Moss RR, Wijesinghe N, Gurvitch R, Tay EL, Thompson C, Webb JG. Transcatheter closure of paravalvular defects using a purpose-specific occluder. *JACC Cardiovasc Interv.* 2010;3:759–765. doi: 10.1016/j.jcin.2010.04.013.
24. Marsan NA, Tops LF, Nihoyannopoulos P, Holman ER, Bax JJ. Real-time three dimensional echocardiography: current and future clinical applications. *Heart.* 2009;95:1881–1890. doi: 10.1136/hrt.2008.151613.
25. Singh P, Manda J, Hsiung MC, Mehta A, Kesanolla SK, Nanda NC, Tsai SK, Wei J, Yin WH. Live/real time three-dimensional transesophageal echocardiographic evaluation of mitral and aortic valve prosthetic paravalvular regurgitation. *Echocardiography.* 2009;26:980–987. doi: 10.1111/j.1540-8175.2009.01022.x.
26. Thaden JJ, Sanon S, Geske JB, Eleid MF, Nijhof N, Malouf JF, Rihal CS, Bruce CJ. echocardiographic and fluoroscopic fusion imaging for procedural guidance: an overview and early clinical experience. *J Am Soc Echocardiogr.* 2016. pii: S0894-7317(16)00046-8. doi: 10.1016/j.echo.2016.01.013. [Epub ahead of print].
27. Hyodo E, Iwata S, Tugcu A, Arai K, Shimada K, Muro T, Yoshikawa J, Yoshiyama M, Gillam LD, Hahn RT, Di Tullio MR, Homma S. Direct measurement of multiple vena contracta areas for assessing the severity of mitral regurgitation using 3D TEE. *JACC Cardiovasc Imaging.* 2012;5:669–676. doi: 10.1016/j.jcmg.2012.03.008.
28. Shanks M, Siebelink HM, Delgado V, van de Veire NR, Ng AC, Sieders A, Schuijff JD, Lamb HJ, Ajmone Marsan N, Westenberg JJ, Kroft LJ, de Roos A, Bax JJ. Quantitative assessment of mitral regurgitation: comparison between three-dimensional transesophageal echocardiography and magnetic resonance imaging. *Circ Cardiovasc Imaging.* 2010;3:694–700. doi: 10.1161/CIRCIMAGING.110.947176.
29. Altiok E, Hamada S, Brehmer K, Kuhr K, Reith S, Becker M, Schröder J, Almalla M, Lehmacher W, Marx N, Hoffmann R. Analysis of procedural effects of percutaneous edge-to-edge mitral valve repair by 2D and 3D echocardiography. *Circ Cardiovasc Imaging.* 2012;5:748–755. doi: 10.1161/CIRCIMAGING.112.974691.
30. Hamilton-Craig C, Strugnell W, Gaikwad N, Ischenko M, Speranza V, Chan J, Neill J, Platts D, Scalia GM, Burstow DJ, Walters DL. Quantitation of mitral regurgitation after percutaneous MitraClip repair: comparison of Doppler echocardiography and cardiac magnetic resonance imaging. *Ann Cardiothorac Surg.* 2015;4:341–351. doi: 10.3978/j.issn.2225-319X.2015.05.03.
31. Hartlage GR, Babaliaros VC, Thourani VH, Hayek S, Chrysohoou C, Ghasemzadeh N, Stillman AE, Clements SD, Oshinski JN, Lerakis S. The role of cardiovascular magnetic resonance in stratifying paravalvular leak severity after transcatheter aortic valve replacement: an observational outcome study. *J Cardiovasc Magn Reson.* 2014;16:93. doi: 10.1186/s12968-014-0093-x.
32. Simprini LA, Goyal P, Codella N, Fieno DS, Afroz A, Mullally J, Cooper M, Wang Y, Finn JP, Devereux RB, Weinsaft JW. Geometry-independent inclusion of basal myocardium yields improved cardiac magnetic resonance agreement with echocardiography and necropsy quantified left-ventricular mass. *J Hypertens.* 2013;31:2069–2076. doi: 10.1097/HJH.0b013e328362d935.
33. Jenkins C, Bricknell K, Hanekom L, Marwick TH. Reproducibility and accuracy of echocardiographic measurements of left ventricular parameters using real-time three-dimensional echocardiography. *J Am Coll Cardiol.* 2004;44:878–886. doi: 10.1016/j.jacc.2004.05.050.

KEY WORDS: Editorials ■ echocardiography ■ multislice computed tomography ■ transcatheter ■ valvular heart disease

## Multimodality Imaging in Transcatheter Mitral Interventions: Buzzword or Modern Age Toolbox?

Omar K. Khalique and Rebecca T. Hahn

*Circ Cardiovasc Imaging*. 2016;9:

doi: 10.1161/CIRCIMAGING.116.005071

*Circulation: Cardiovascular Imaging* is published by the American Heart Association, 7272 Greenville Avenue, Dallas, TX 75231

Copyright © 2016 American Heart Association, Inc. All rights reserved.

Print ISSN: 1941-9651. Online ISSN: 1942-0080

The online version of this article, along with updated information and services, is located on the World Wide Web at:

<http://circimaging.ahajournals.org/content/9/6/e005071>

**Permissions:** Requests for permissions to reproduce figures, tables, or portions of articles originally published in *Circulation: Cardiovascular Imaging* can be obtained via RightsLink, a service of the Copyright Clearance Center, not the Editorial Office. Once the online version of the published article for which permission is being requested is located, click Request Permissions in the middle column of the Web page under Services. Further information about this process is available in the [Permissions and Rights Question and Answer](#) document.

**Reprints:** Information about reprints can be found online at:  
<http://www.lww.com/reprints>

**Subscriptions:** Information about subscribing to *Circulation: Cardiovascular Imaging* is online at:  
<http://circimaging.ahajournals.org/subscriptions/>